P6 SCALING TIPS

Knowing when to replace your tips is essential, as tip wear will significantly reduce scaler performance – as it alters the ultrasonic frequency.

Each tip is designed for different cleaning needs, from coarse to fine depuration, for tackling both large deposits and interdental areas.

Up to 1 mm: Optimum efficiency


1-2 mm: Time to re-order

Over 2 mm: Time to dispose

PLACE YOUR SCALER TIP OVER THE RELEVANT IMAGE TO CHECK YOUR TIP MEASUREMENT

Universal (Coarse)


U6S01



For coarse depuration of supragingival calculus.

Universal (Fine)


U6G3



For fine depuration of supragingival calculus.

Perio 1P

U6PD3




For removal of subgingival deposits.

Reorder new tips at www.im3vet.eu

Please use the correct wrench supplied with the tip, and make sure it is fully tightened.

iM3® | THE GLOBAL NAME IN VETERINARY DENTISTRY

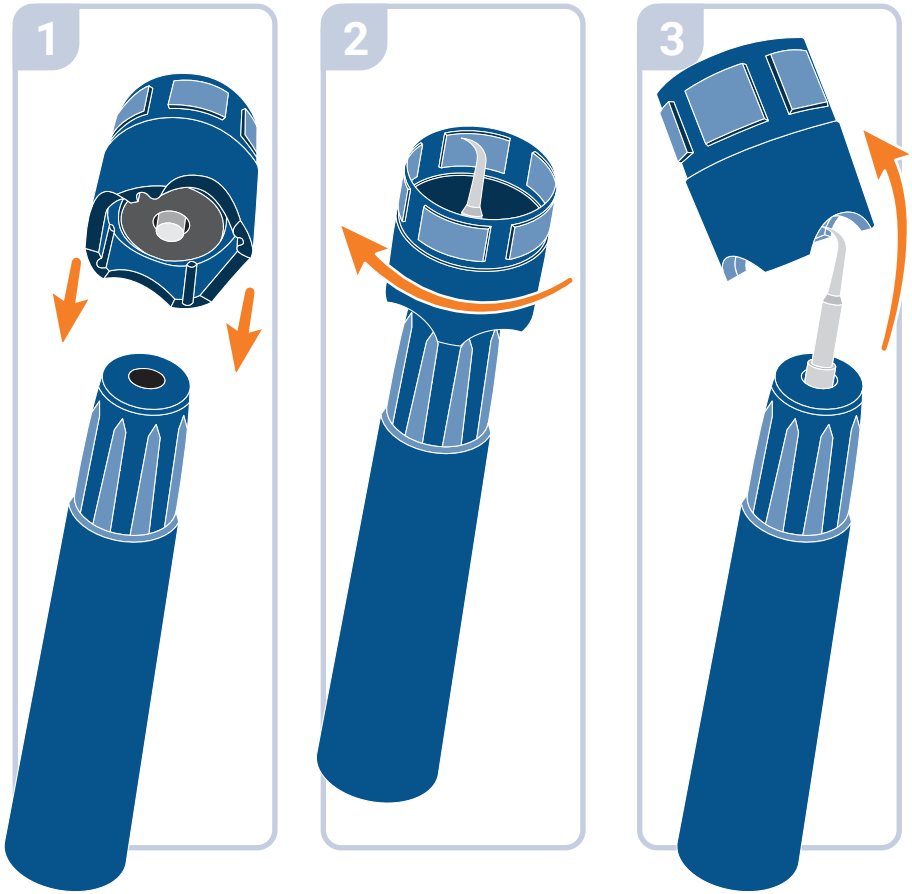

HOW TO INSTALL A P6 SCALING TIP

Using the torque wrench, insert the scaling tip into the handpiece coupling.

Exercise light pressure, stopping immediately when the wrench indicates that the preset torque is reached.

Avoid over-tightening by continuing past the indicated torque.

"I am seeing "Error 6" / my scaler light is flashing - why is this?"

First check that your scaler tip is correctly attached to the scaler coupling. If the issue persists, replace the scaler tip with a new iM3 tip.

If this fails to solve your issue, please contact us at: support@im3dental.com

Reorder new tips at www.im3vet.eu

Please use the correct wrench supplied with the tip, and make sure it is fully tightened.

iM3® | THE GLOBAL NAME IN VETERINARY DENTISTRY